


































sales@panswmed.com
 pan-sw@hotmail.com
 Tel: 86-20-28961025
 Skype:panmedical; dianapansw






PANSW Part code	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10001A		Philips 78352A, M1165A, MerlinViridia 24, CMS 24 M3/M4, M1175A, M1350B, M1205A, M1350A, M1353A, 8030A, 8040A		Use with Abbott/Medex IBP transducer
IBP-10001B				Use with Utah IBP transducer
IBP-10001C				Use with Edward IBP transducer
IBP-10001D				Use with BD IBP transducer
IBP-10001E				Use with Argon IBP transducer
IBP-10001F				Use with B. Bruan IBP transducer
IBP-10001G				


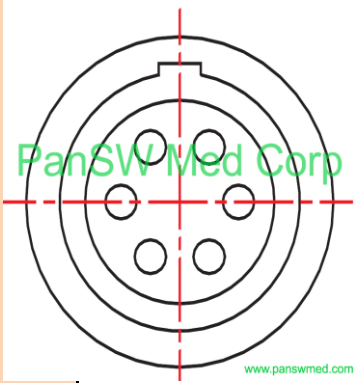
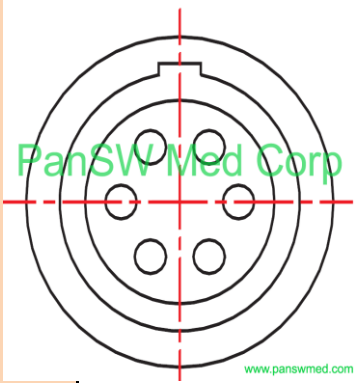

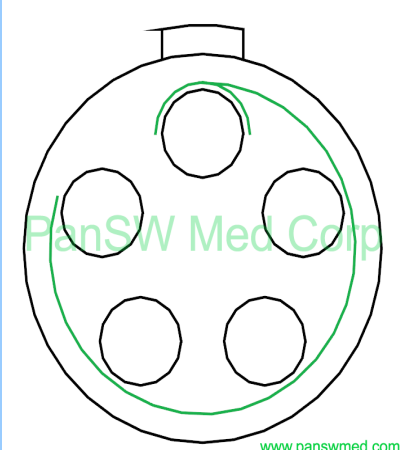
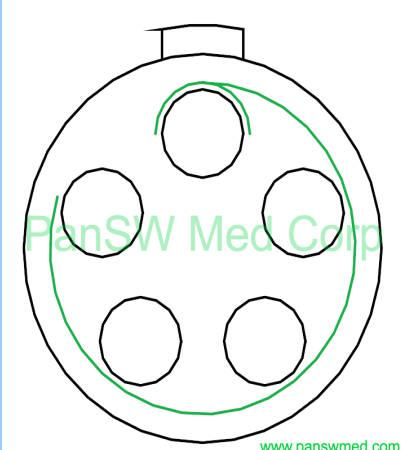
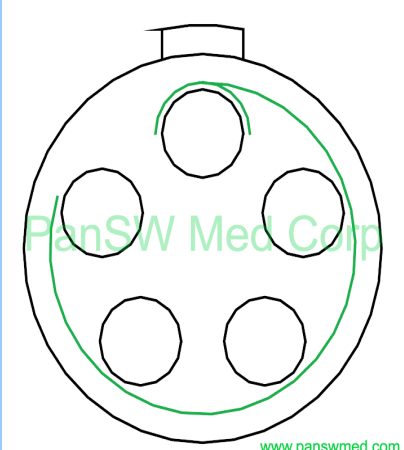
IBP-10001H				Use with Medex Logical
PANSW Part number	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10002A		Siemens/Darger : SC6002XL, 7000, SC8000, SC9000XL		Use with Abbott/Medex IBP transducer
IBP-10002B				Use with Utah IBP transducer
IBP-10002C				Use with Edward IBP transducer
IBP-10002D				Use with BD IBP transducer
IBP-10002E				Use with Argon IBP transducer
IBP-10002F				Use with B. Bruan IBP transducer
PANSW Part number	Original part number		Brands& compatibilities	Pictures
IBP-10003A		Spacelabs monitors (for		Use with Abbott/Medex IBP transducer
IBP-10003B				Use with Utah IBP transducer
IBP-10003C				Use with Edward IBP


IBP-10003C		MONITORS (101 module 90496 requires adapter cable); original part number: 700-0028-00; Mindray: PM7000, 8000, 9000, 6201.		transducer
IBP-10003D				Use with BD IBP transducer
IBP-10003E				Use with Argon IBP transducer
IBP-10003F				Use with B.Bruan IBP transducer
IBP-10003G				
IBP-10003SF				
PANSW Part number	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10004A	2021196-001/2021196-002			Use with Abbott/Medex IBP transducer
IBP-100042DA				Use with Abbott/Medex IBP transducer
IBP-10004B	2016997-001/2016997-002			Use with Utah IBP transducer
IBP-100042DB				Use with Utah IBP transducer



		GE Marquette; GE Solar, Dash, Eagle, Tram		
IBP-10004C	2021197-001/2021197-002			Use with Edward IBP transducer
IBP-10004D	2016995-001/2016995-002			Use with BD IBP transducer
IBP-10004E				Use with Argon IBP transducer
IBP-10004F	GE part number: 22339301			Use with B. Brua IBP transducer
IBP-10004G				
PANSW Part number	Original part number	Brands & compatibilities	Pictures	Descriptions
IBP-10005A		GE datex; Airshield, Burdick, Kone		Use with Abbott/Medex IBP transducer
IBP-10005B				Use with Utah IBP transducer
IBP-10005C				Use with Edward IBP transducer
IBP-10005D				Use with BD IBP transducer
IBP-10005E				Use with Argon IBP transducer




IBP-10005F				Use with B. Brua IBP transducer
IBP-10005G				Use with USB connector
PANSW Part number	Original part number	Brands& compatibilities	Pictures	Descriptions
IBP-10006A		Nihon Kohden IPB cable; BSM-2300 Lifescop i/L; BSM-4100 Lifescop P; BSM-5100 Lifescop A; BSM-9510 Lifescop M; BSM-9800 Lifescop S;		Use with Abbott/Medex IBP transducer
IBP-10006B				Use with Utah IBP transducer
IBP-10006C	JP-920P			Use with Edward IBP transducer
IBP-10006D	JP-900P			Use with BD IBP transducer
IBP-10006E				Use with Argon IBP transducer
IBP-10006F				Use with B. Brua IBP transducer
IBP-10007A				Use with Abbott/Medex IBP transducer
IBP-10007B				Use with Utah IBP transducer

IBP-10007C		Siemens Medical: Sirecust 700, Sirecust 630 Sirecust 400- 1281, SC8000		Use with Edward IBP transducer
IBP-10007D				Use with BD IBP transducer
IBP-10007E				Use with Argon IBP transducer
IBP-10007F				Use with B. Brua IBP transducer
IBP-10008A				Use with Abbott/Medex IBP transducer
IBP-10008B				Use with Utah IBP transducer
IBP-10008C		datascope IBP cable		Use with Edward IBP transducer
IBP-10008D				Use with BD IBP transducer
IBP-10008E				Use with Argon IBP transducer
IBP-10008F				Use with B. Brua IBP transducer
IBP-10009A				Use with Abbott/Medex IBP transducer


IBP-10009B		Colin IBP cable		Use with Utah IBP transducer
IBP-10009C				Use with Edward IBP transducer
IBP-10009D				Use with BD IBP transducer
IBP-10009E				Use with Argon IBP transducer
IBP-10009F				Use with B. Brua IBP transducer
IBP-10010A		CSI IBP cable		Use with Abbott/Medex IBP transducer
IBP-10010B				Use with Utah IBP transducer
IBP-10010C				Use with Edward IBP transducer
IBP-10010D				Use with BD IBP transducer
IBP-10010E				Use with Argon IBP transducer
IBP-10010F				Use with B. Brua IBP transducer

IBP-10011A		Mindray IBP cable		Use with Abbott/Medex IBP transducer
IBP-10011B				Use with Utah IBP transducer
IBP-10011C				Use with Edward IBP transducer
IBP-10011D				Use with BD IBP transducer
IBP-10011E				Use with Argon IBP transducer
IBP-10011F				Use with B. Brua IBP transducer
IBP-10012A				Use with Abbott/Medex IBP transducer
IBP-10012B				Use with Utah IBP transducer
IBP-10012C		Fukuda IBP cable		Use with Edward IBP transducer
IBP-10012D				Use with BD IBP transducer
IBP-10012E				Use with Argon IBP transducer

IBP-10012F				Use with B. Brua IBP transducer	
IBP-10013A				Use with Abbott/Medex IBP transducer	
IBP-10013B				Use with Utah IBP transducer	
IBP-10013C			<p>biolight IBP cable</p>		Use with Edward IBP transducer
IBP-10013D					Use with BD IBP transducer
IBP-10013E					Use with Argon IBP transducer
IBP-10013F					Use with B. Brua IBP transducer
IBP-10014A					
IBP-10014B			Use with Utah IBP transducer		
IBP-10014C		<p>FUKUDA IBP cable</p>			Use with Edward IBP transducer
IBP-10014D					Use with BD IBP transducer
IBP-10014E					Use with Argon IBP transducer

IBP-10014F				Use with B. Brua IBP transducer
IBP-10015A				drager dual connector adapter cable
IBP-10016A				Use with Abbott/Medex IBP transducer
IBP-10016B				Use with Utah IBP transducer
IBP-10016C		Nihon kohden IBP cable		Use with Edward IBP transducer
IBP-10016D				Use with BD IBP transducer
IBP-10016E				Use with Argon IBP transducer
IBP-10016F				Use with B. Brua IBP transducer
IBP-10017A		datascope IBP cable		Use with Abbott/Medex IBP transducer
IBP-10017B				Use with Utah IBP transducer

IBP-10017C				Use with Edward IBP transducer
IBP-10017D				Use with BD IBP transducer
IBP-10017E				Use with Argon IBP transducer
IBP-10017F				Use with B. Brua IBP transducer
IBP-10018A				Use with Abbott/Medex IBP transducer
IBP-10018B				Use with Utah IBP transducer
IBP-10018C				Use with Edward IBP transducer
IBP-10018D		Kontron IBP cable Minimon 7131-7136, BC-KTN-AG BC-KTN-BB BC-KTN-BD BC-KTN-ED BC-KTN-MX BC-KTN-UT Fetalmon 2A, 2B Fetalogic 4000, Fetasonde 5, 5A, 5B K2000 Ballon Pump; KAAT II Module 10-7286, Supermon		Use with BD IBP transducer
IBP-10018E				Use with Argon IBP transducer
IBP-10018F				Use with B. Brua IBP transducer
IBP-10019A		MENNEN IBP CABLES; ENVOY, VITALOGIC		Use with Abbott/Medex IBP transducer

IBP-10019B				Use with Utah IBP transducer
IBP-10019C				Use with Edward IBP transducer
IBP-10019D				Use with BD IBP transducer
IBP-10019E				Use with Argon IBP transducer
IBP-10019F				Use with B. Brua IBP transducer
IBP-10020A		REDEL 6 PINS SINGLE NOTCH		Use with Abbott/Medex IBP transducer
IBP-10020B				Use with Utah IBP transducer
IBP-10020C				Use with Edward IBP transducer
IBP-10020D				Use with BD IBP transducer
IBP-10020E				Use with Argon IBP transducer
IBP-10020F				Use with B. Brua IBP transducer